


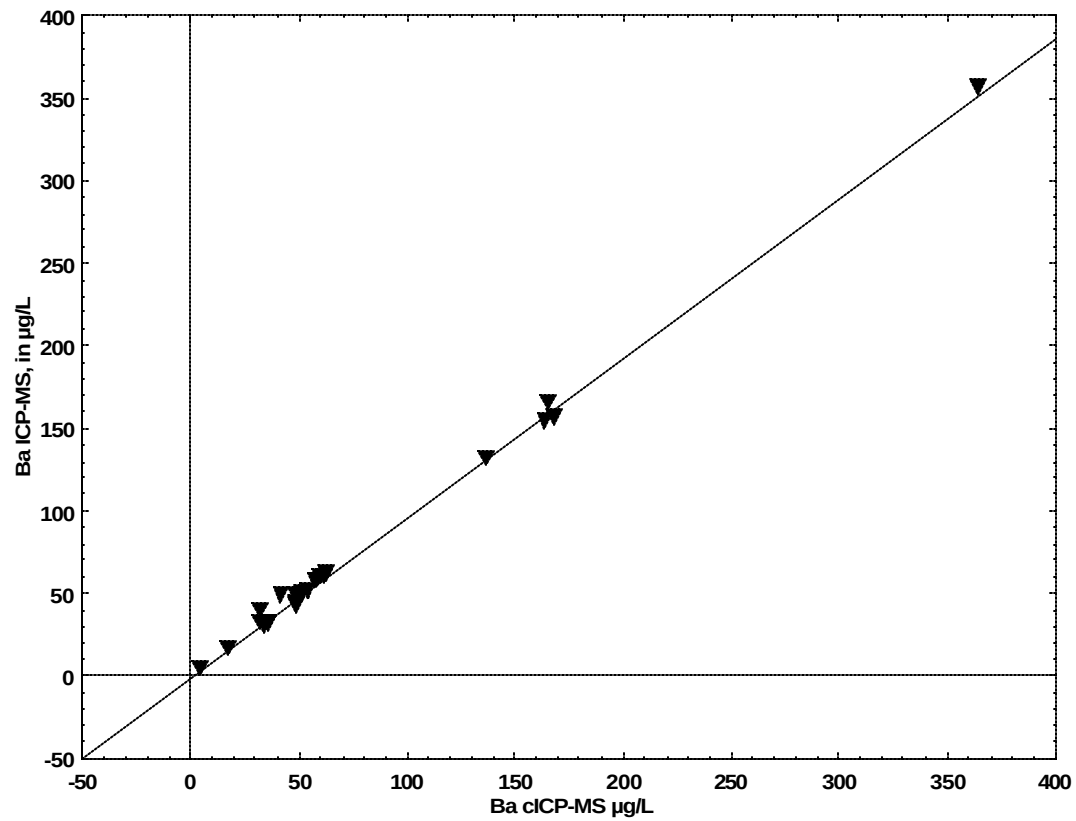

LINEAR REGRESSION EQUATION

$$\text{Ba ICP-MS, in } \mu\text{g/L} = -1.493 + .97 * \text{Ba clCP-MS } \mu\text{g/L}; R^2 = .998$$

Confidence Intervals Ba ICP-MS, in µg/L vs. Ba clCP-MS µg/L

	Coefficient	95% Lower	95% Upper
Intercept	-1.493	-3.517	.531
Ba clCP-MS µg/L	.970	.951	.990