


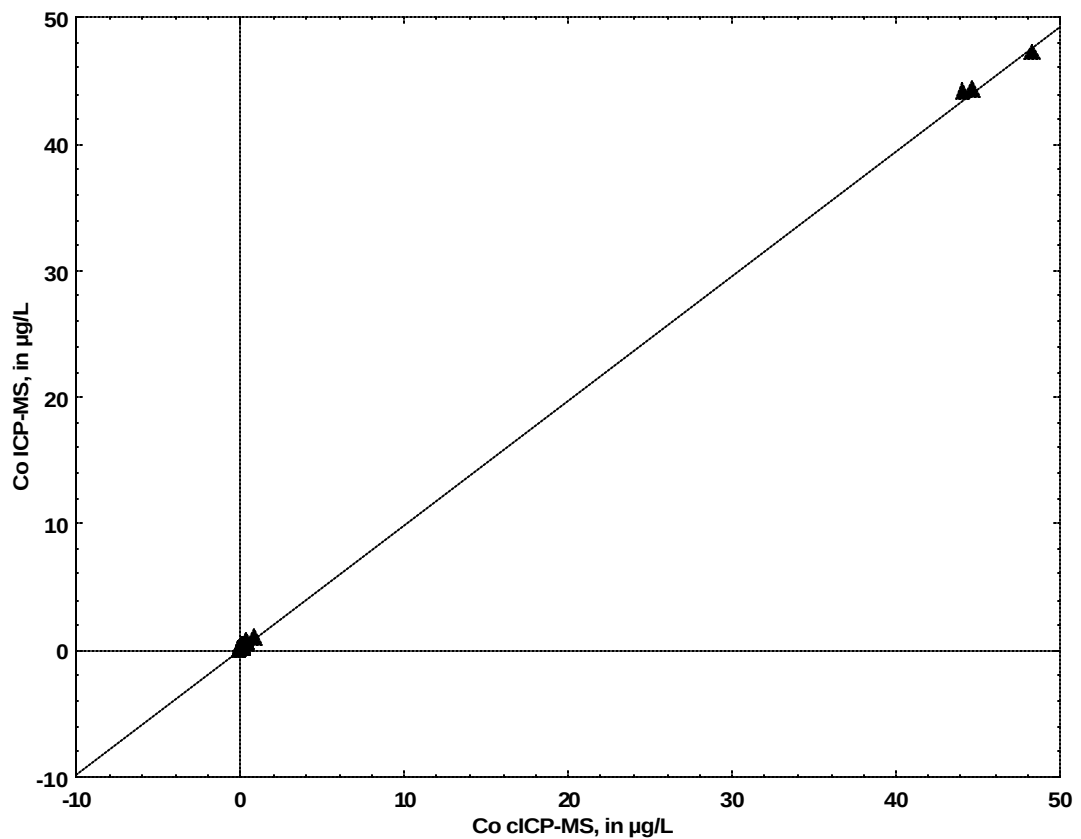

LINEAR REGRESSION EQUATION

$$\text{Co ICP-MS, in } \mu\text{g/L} = .018 + .986 * \text{Co cICP-MS, in } \mu\text{g/L}; R^2 = 1$$

Confidence Intervals Co ICP-MS, in µg/L vs. Co cICP-MS, in µg/L

	Coefficient	95% Lower	95% Upper
Intercept	.018	-.049	.085
Co cICP-MS, in µg/L	.986	.981	.990