


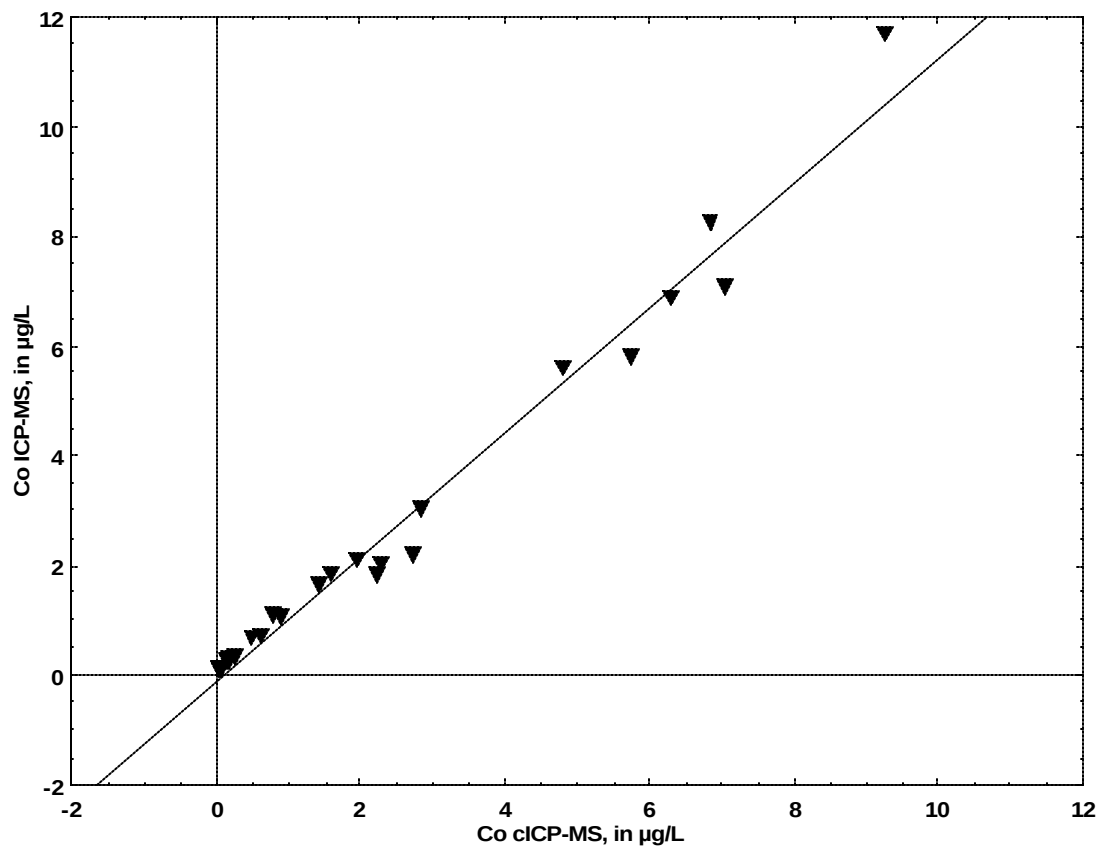

LINEAR REGRESSION EQUATION

Co ICP-MS, in µg/L = $-.127 + 1.137 \cdot \text{Co clCP-MS, in } \mu\text{g/L}$; $R^2 = .979$

Confidence Intervals Co ICP-MS, in µg/L vs. Co clCP-MS, in µg/L

	Coefficient	95% Lower	95% Upper
Intercept	-.127	-.382	.127
Co clCP-MS, in µg/L	1.137	1.065	1.208