


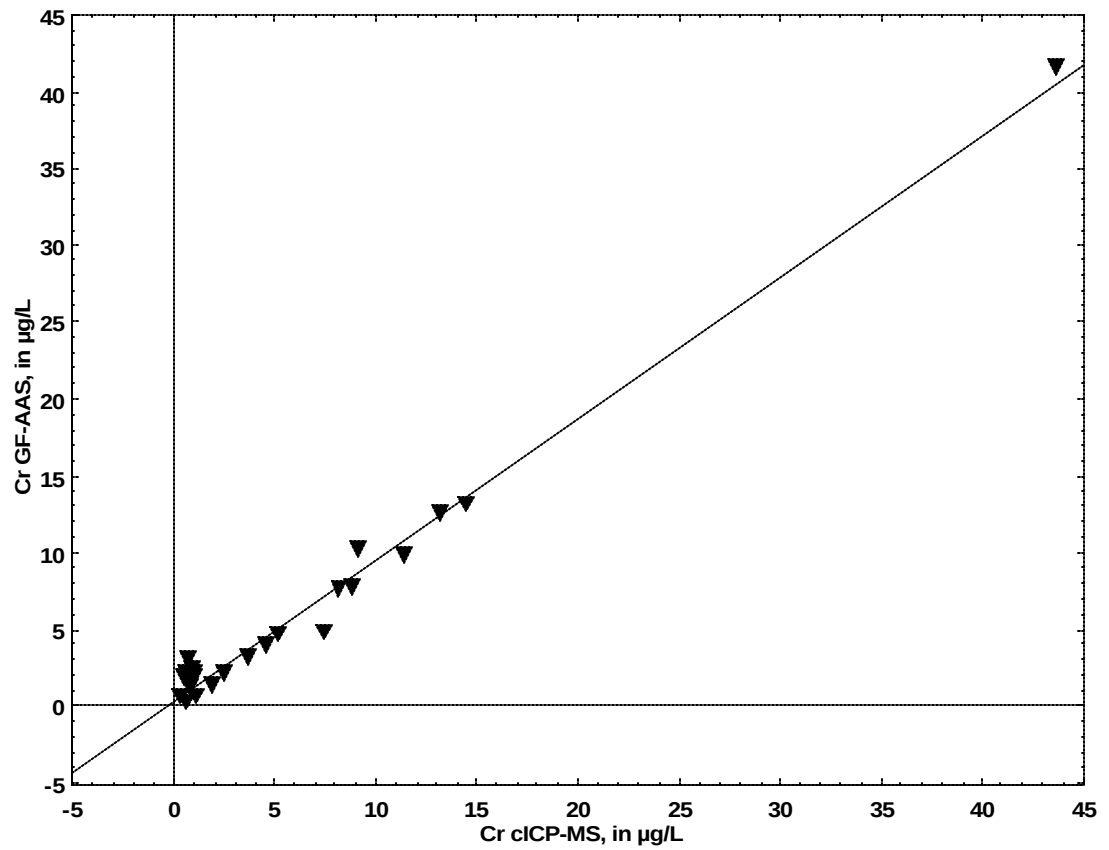

LINEAR REGRESSION EQUATION

$$\text{Cr GF-AAS, in } \mu\text{g/L} = .232 + .921 * \text{Cr cICP-MS, in } \mu\text{g/L}; R^2 = .986$$

Confidence Intervals Cr GF-AAS, in µg/L vs. Cr cICP-MS, in µg/L

	Coefficient	95% Lower	95% Upper
Intercept	.232	-.274	.738
Cr cICP-MS, in µg/L	.921	.874	.969