


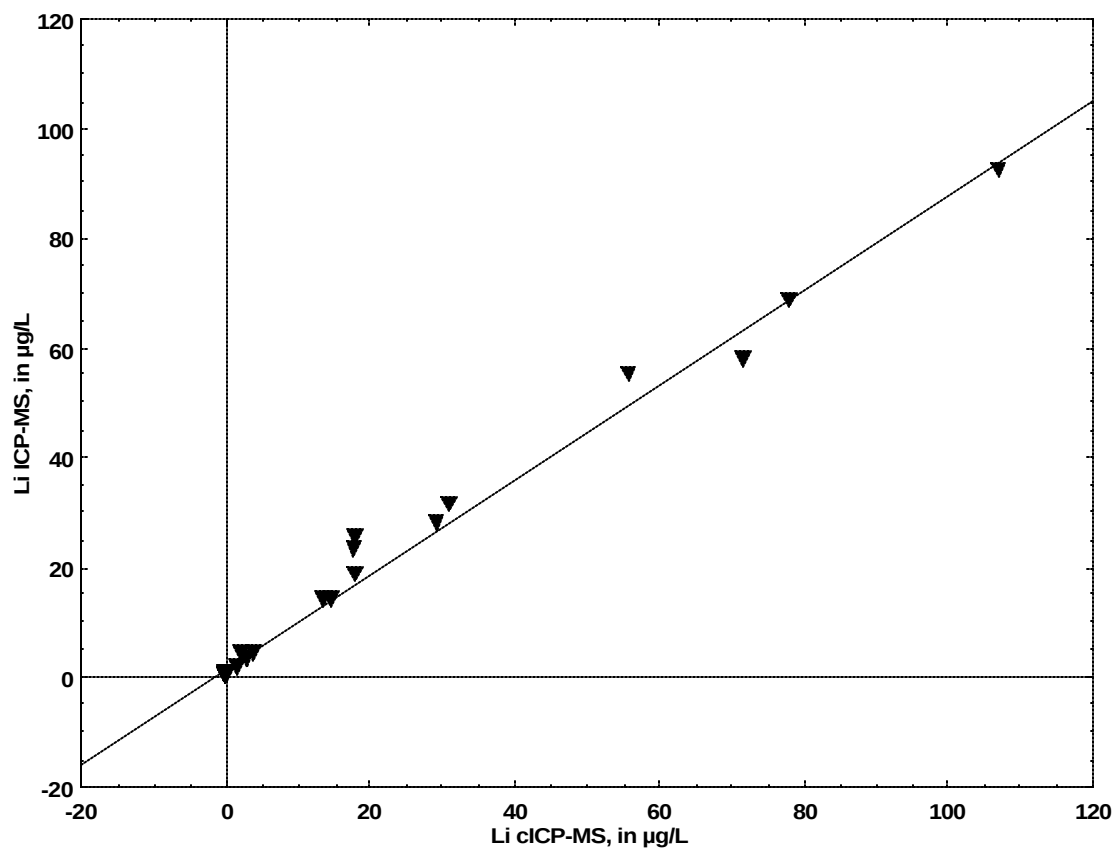

LINEAR REGRESSION EQUATION

Li ICP-MS, in µg/L = 1.472 + .863 * Li cICP-MS, in µg/L; $R^2 = .987$

Confidence Intervals Li ICP-MS, in µg/L vs. Li cICP-MS, in µg/L

	Coefficient	95% Lower	95% Upper
Intercept	1.472	.018	2.926
Li cICP-MS, in µg/L	.863	.821	.906