


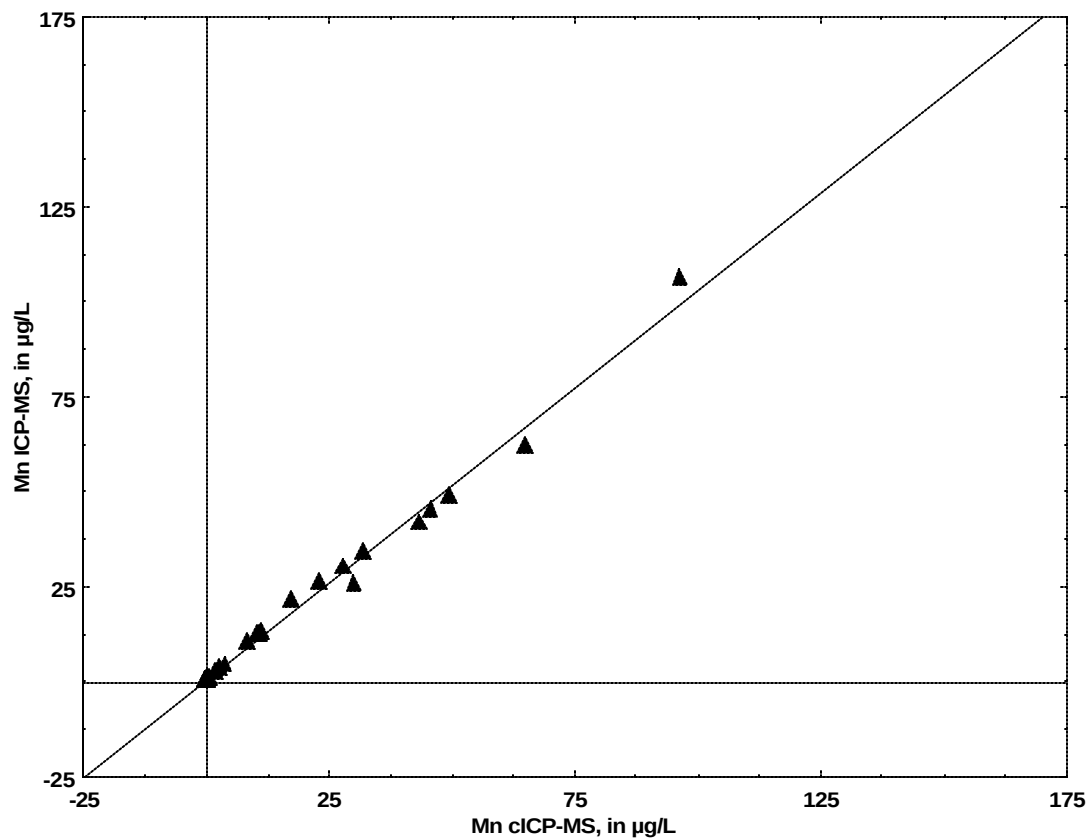

LINEAR REGRESSION EQUATION

$$\text{Mn ICP-MS, in } \mu\text{g/L} = .082 + 1.026 * \text{Mn cICP-MS, in } \mu\text{g/L}; R^2 = .991$$

Confidence Intervals Mn ICP-MS, in µg/L vs. Mn cICP-MS, in µg/L

	Coefficient	95% Lower	95% Upper
Intercept	.082	-1.256	1.420
Mn cICP-MS, in µg/L	1.026	.983	1.069