


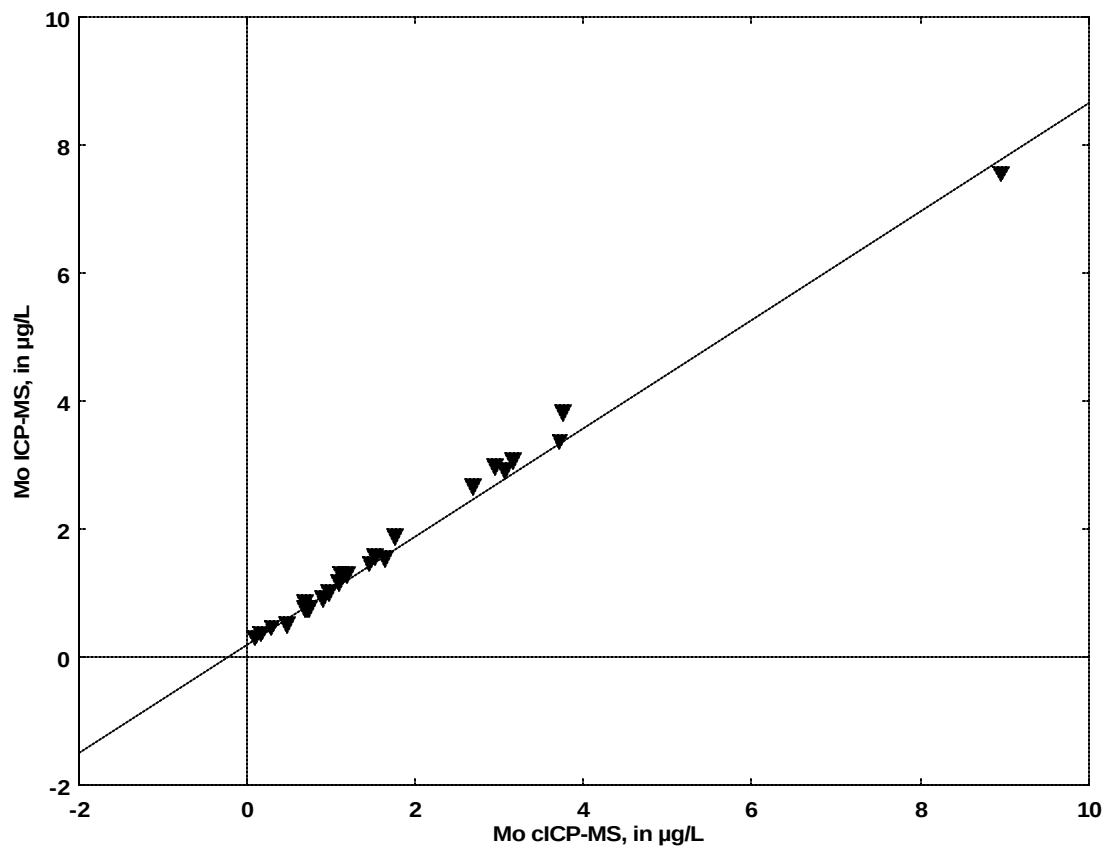

LINEAR REGRESSION EQUATION

$$\text{Mo ICP-MS, in } \mu\text{g/L} = .202 + .847 * \text{Mo cICP-MS, in } \mu\text{g/L}; R^2 = .993$$

Confidence Intervals
Mo ICP-MS, in µg/L vs. Mo cICP-MS, in µg/L

	Coefficient	95% Lower	95% Upper
Intercept	.202	.119	.286
Mo cICP-MS, in µg/L	.847	.815	.879