


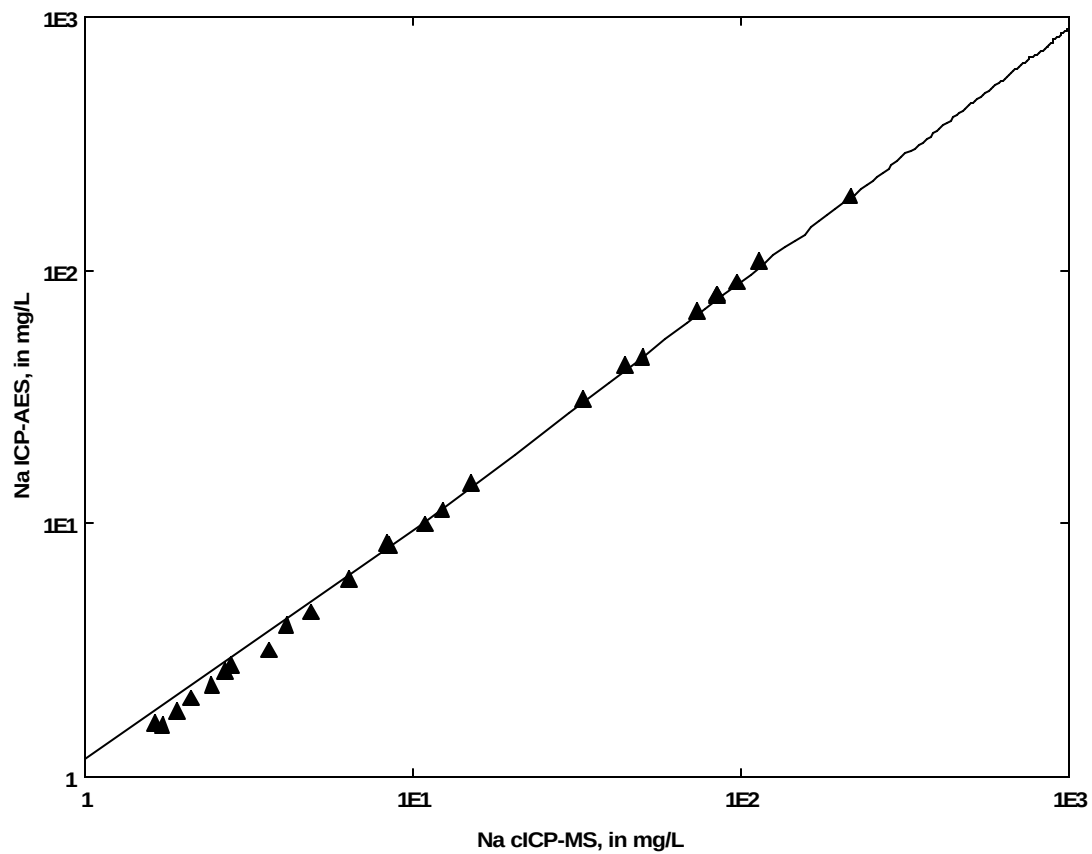

LINEAR REGRESSION EQUATION

Na ICP-AES, in mg/L = .273 + .906 * Na cICP-MS, in mg/L; $R^2 = 1$

Confidence Intervals Na ICP-AES, in mg/L vs. Na cICP-MS, in mg/L

	Coefficient	95% Lower	95% Upper
Intercept	.273	-.263	.810
Na cICP-MS, in mg/L	.906	.898	.915