


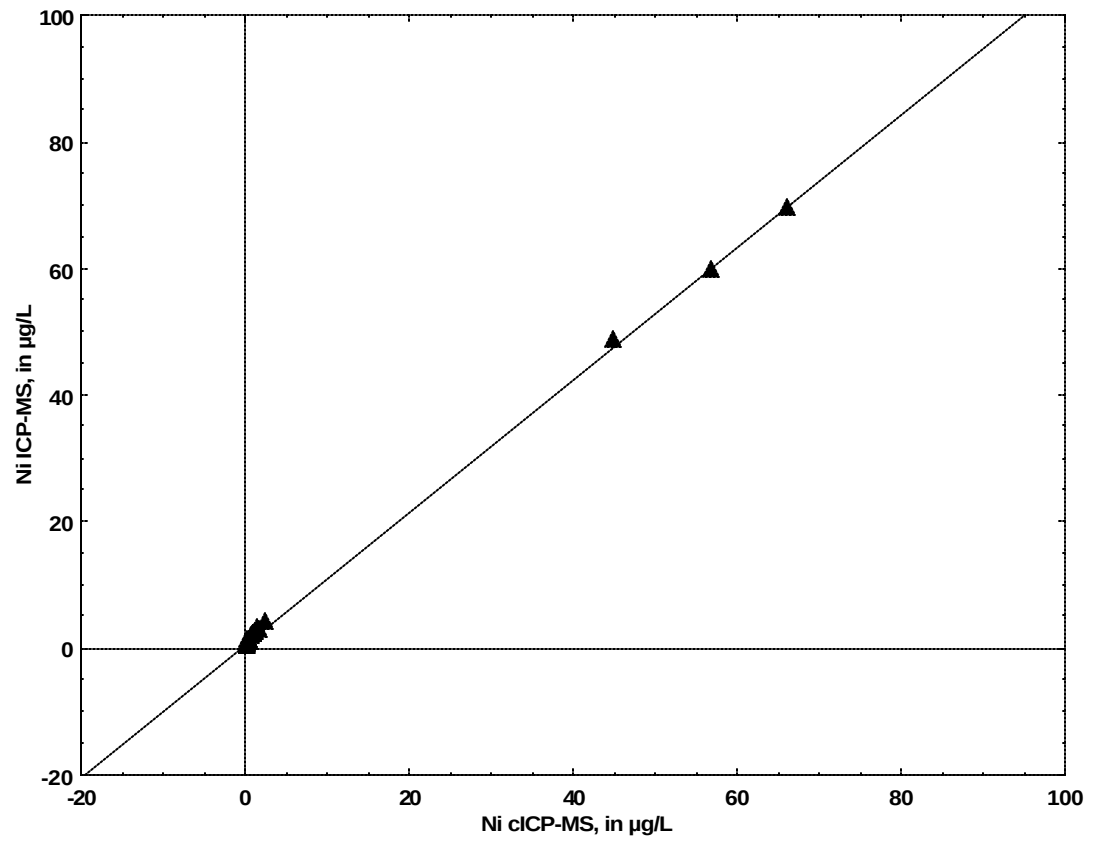

LINEAR REGRESSION EQUATION

$$\text{Ni ICP-MS, in } \mu\text{g/L} = .494 + 1.045 * \text{Ni clCP-MS, in } \mu\text{g/L}; R^2 = .999$$

Confidence Intervals Ni ICP-MS, in µg/L vs. Ni clCP-MS, in µg/L

	Coefficient	95% Lower	95% Upper
Intercept	.494	.285	.704
Ni clCP-MS, in µg/L	1.045	1.035	1.056