


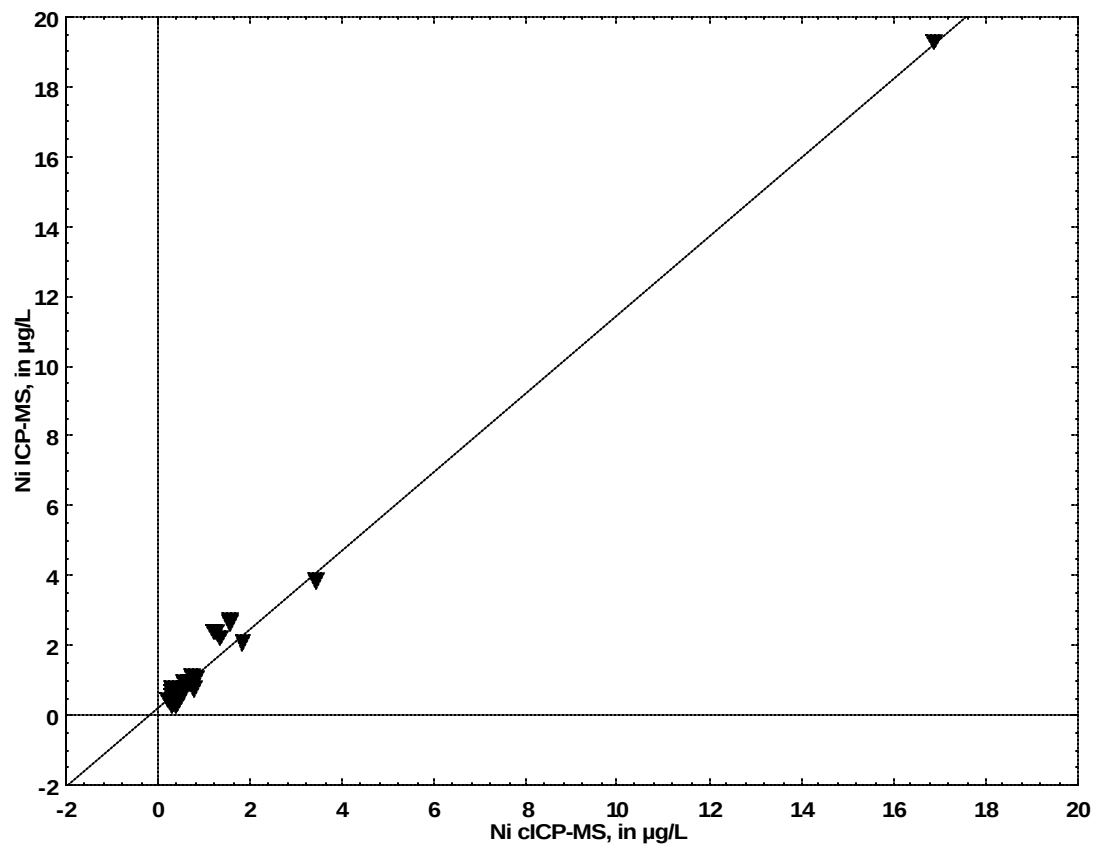

LINEAR REGRESSION EQUATION

$$\text{Ni ICP-MS, in } \mu\text{g/L} = .188 + 1.128 * \text{Ni clCP-MS, in } \mu\text{g/L}; R^2 = .99$$

Confidence Intervals Ni ICP-MS, in µg/L vs. Ni clCP-MS, in µg/L

	Coefficient	95% Lower	95% Upper
Intercept	.188	.016	.360
Ni clCP-MS, in µg/L	1.128	1.080	1.176