


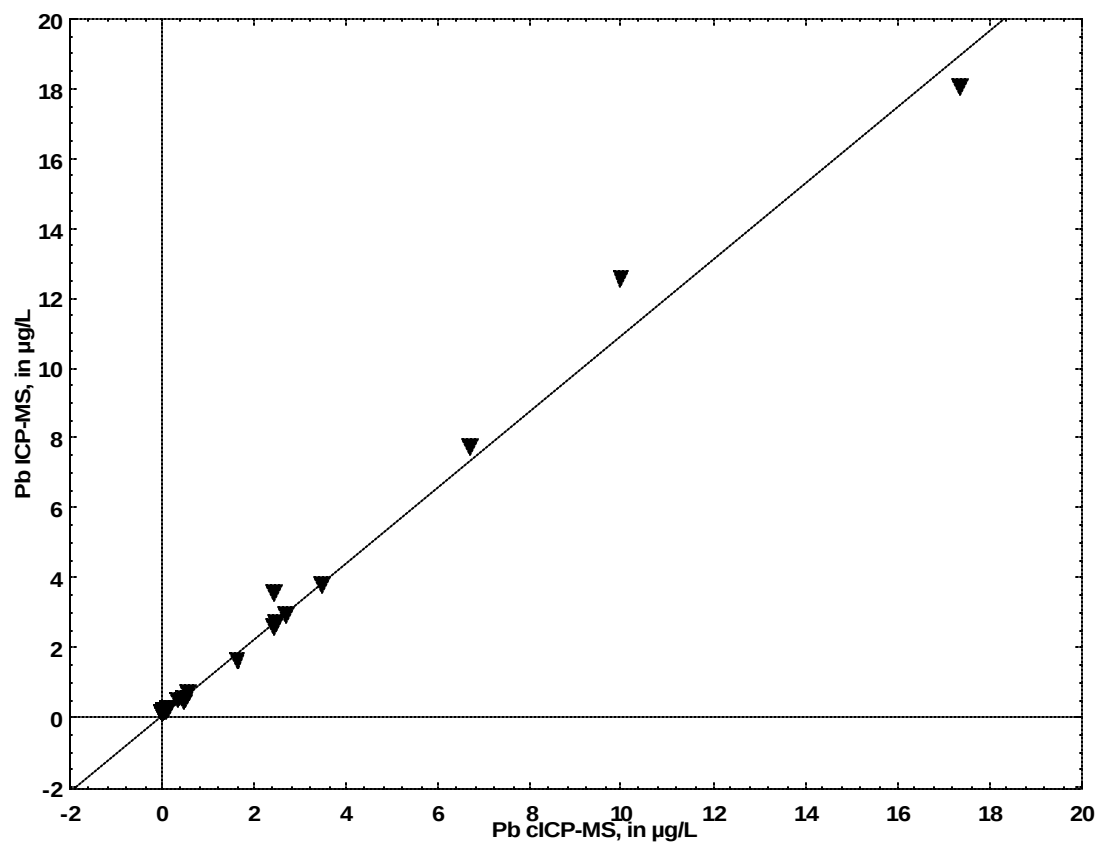

LINEAR REGRESSION EQUATION

Pb ICP-MS, in µg/L = .039 + 1.089 * Pb clCP-MS, in µg/L; $R^2 = .99$

Confidence Intervals Pb ICP-MS, in µg/L vs. Pb clCP-MS, in µg/L

	Coefficient	95% Lower	95% Upper
Intercept	.039	-.167	.244
Pb clCP-MS, in µg/L	1.089	1.043	1.135