


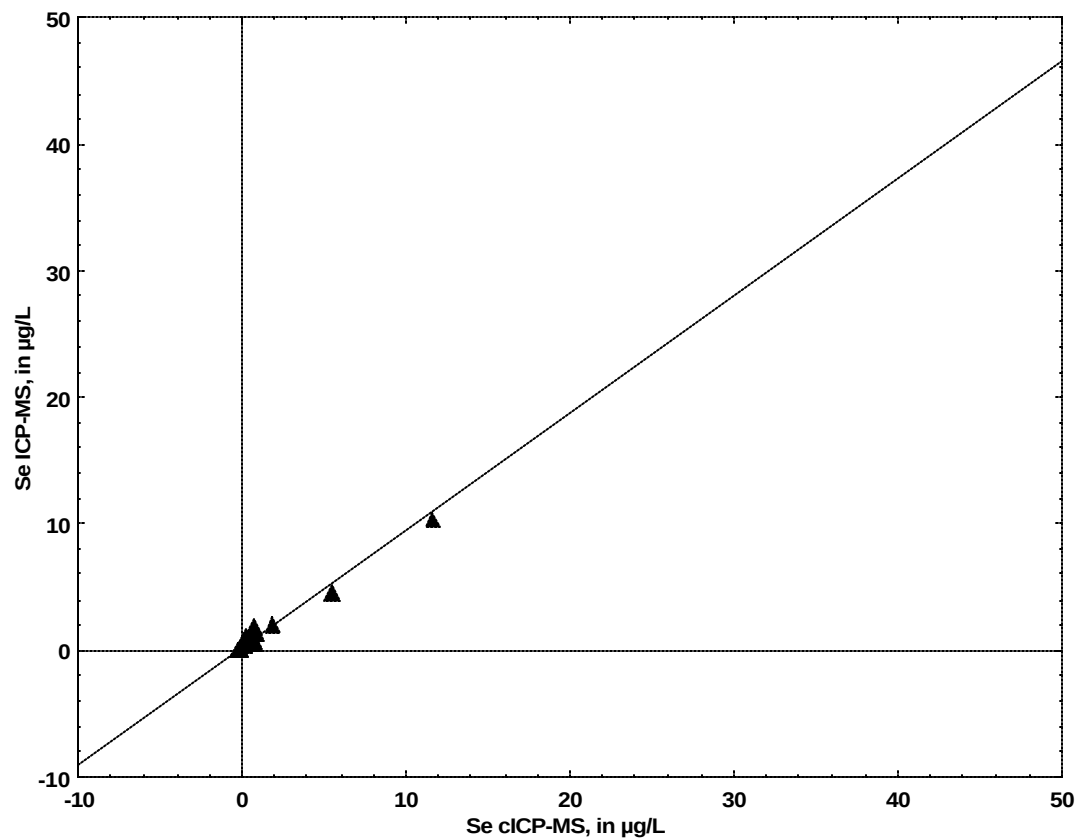

LINEAR REGRESSION EQUATION

$$\text{Se ICP-MS, in } \mu\text{g/L} = .134 + .929 * \text{Se cICP-MS, in } \mu\text{g/L}; R^2 = .998$$

Confidence Intervals Se ICP-MS, in µg/L vs. Se cICP-MS, in µg/L

	Coefficient	95% Lower	95% Upper
Intercept	.134	-.035	.303
Se cICP-MS, in µg/L	.929	.913	.944