


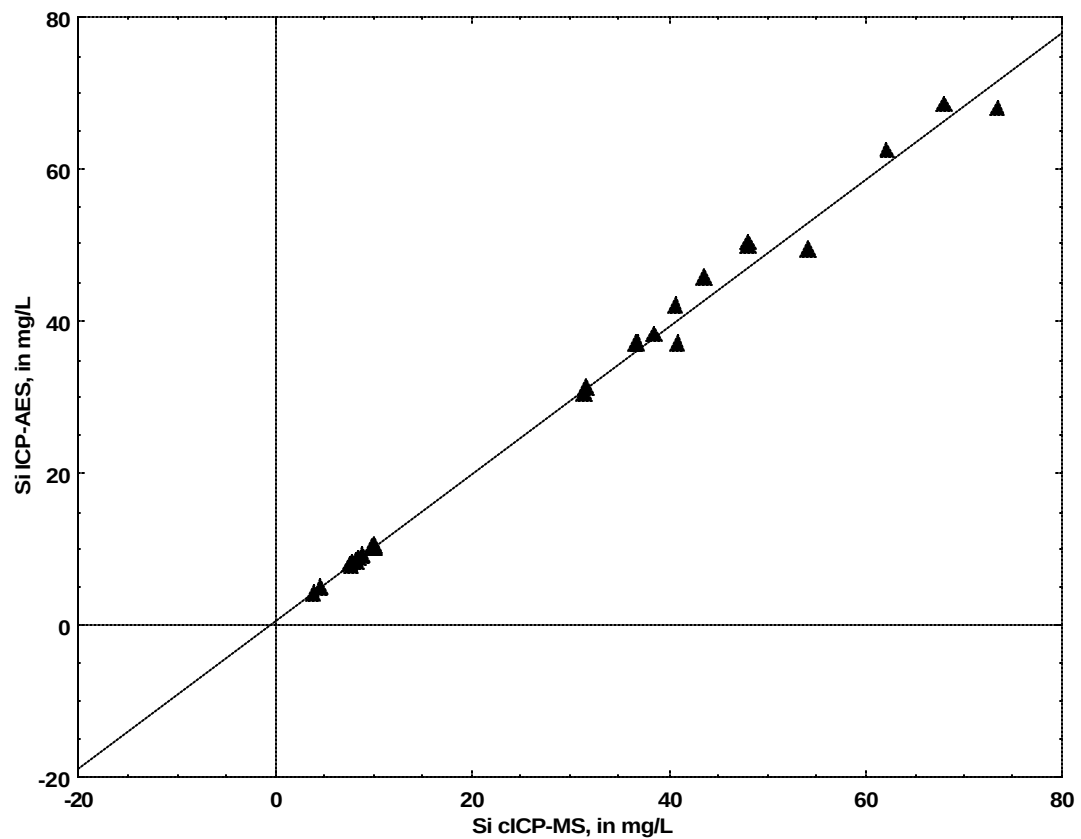

LINEAR REGRESSION EQUATION

$$\text{Si ICP-AES, in mg/L} = .339 + .971 * \text{Si cICP-MS, in mg/L}; R^2 = .993$$

Confidence Intervals Si ICP-AES, in mg/L vs. Si cICP-MS, in mg/L

	Coefficient	95% Lower	95% Upper
Intercept	.339	-.890	1.567
Si cICP-MS, in mg/L	.971	.937	1.005