


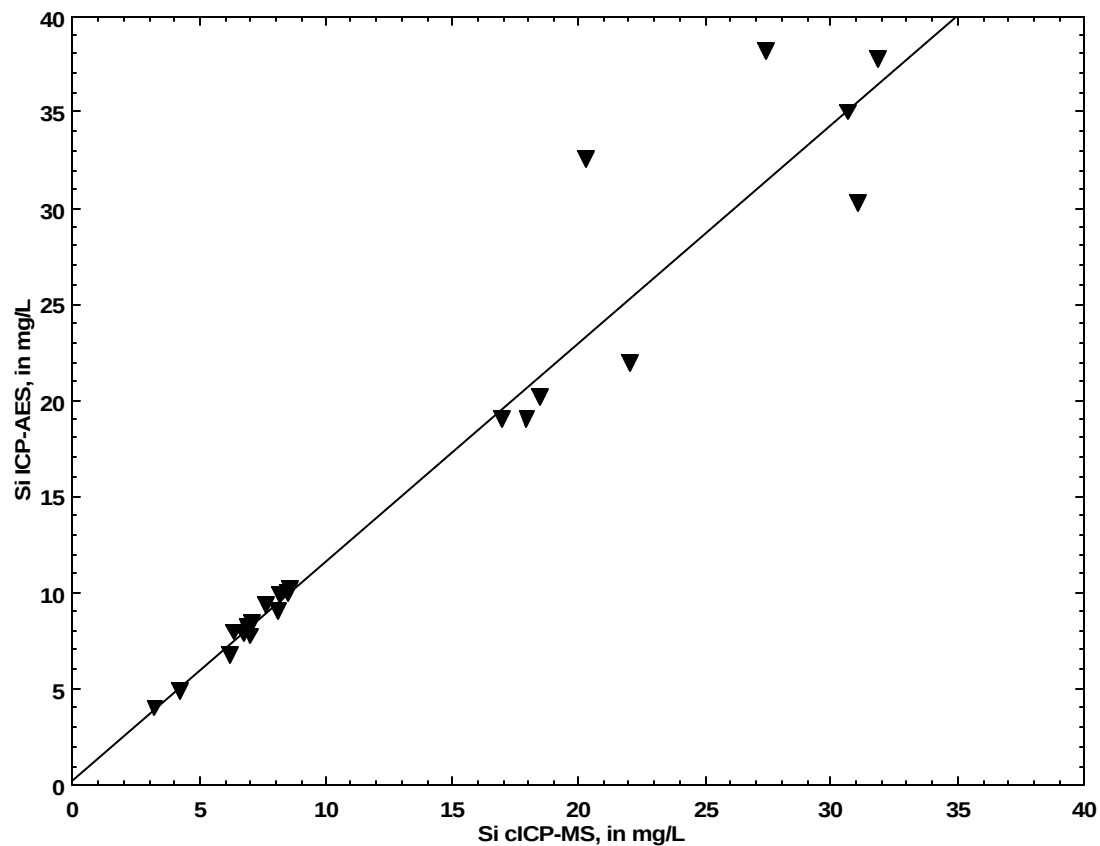

**LINEAR REGRESSION EQUATION**

$$\text{Si ICP-AES, in mg/L} = .238 + 1.136 * \text{Si cICP-MS, in mg/L}; R^2 = .946$$

**Confidence Intervals**  
Si ICP-AES, in mg/L vs. Si cICP-MS, in mg/L

|                     | Coefficient | 95% Lower | 95% Upper |
|---------------------|-------------|-----------|-----------|
| Intercept           | .238        | -1.999    | 2.475     |
| Si cICP-MS, in mg/L | 1.136       | 1.014     | 1.259     |