


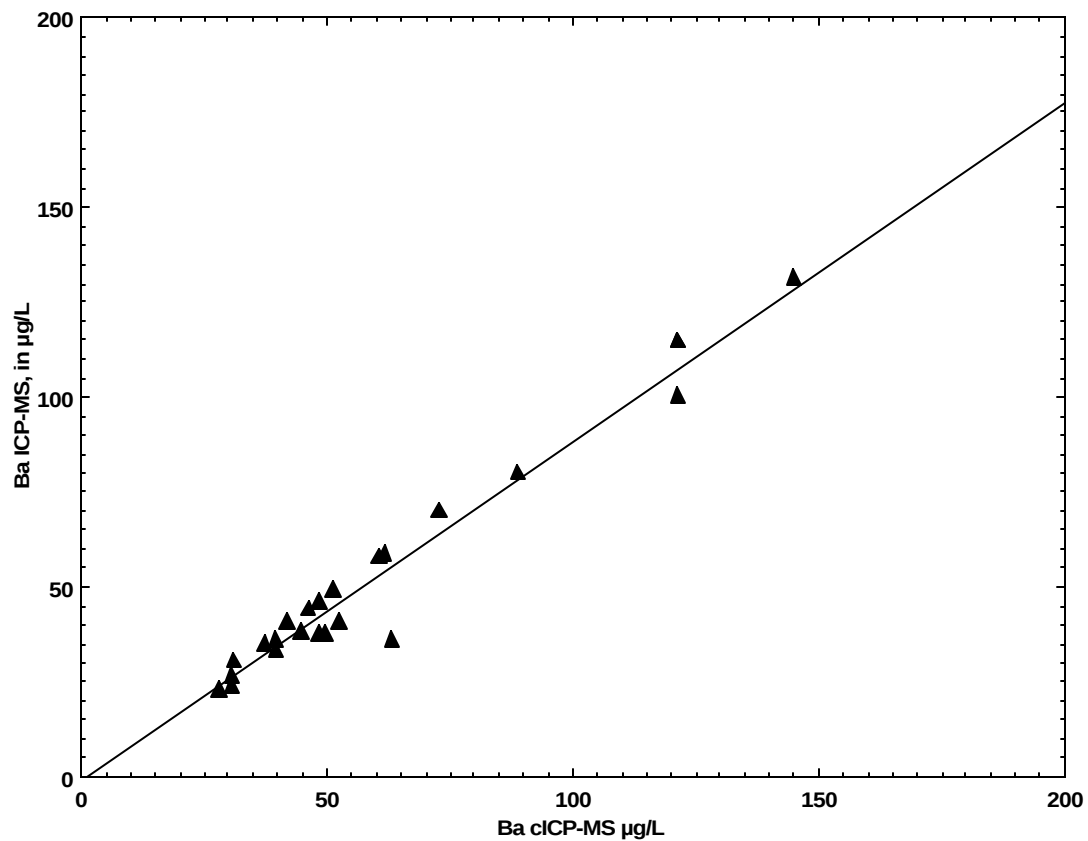

LINEAR REGRESSION EQUATION

$$\text{Ba ICP-MS, in } \mu\text{g/L} = -1.117 + .891 * \text{Ba clCP-MS } \mu\text{g/L}; R^2 = .977$$

Confidence Intervals Ba ICP-MS, in µg/L vs. Ba clCP-MS µg/L

	Coefficient	95% Lower	95% Upper
Intercept	-1.117	-5.782	3.548
Ba clCP-MS µg/L	.891	.832	.949